

## 2657A High Power System SourceMeter® SMU Instrument

### DATASHEET




The 2657A is a high voltage, high power, low current source measure unit (SMU) instrument that delivers unprecedented power, precision, speed, flexibility, and ease of use to improve productivity in R&D, production test, and reliability environments. The 2657A is designed specifically for characterizing and testing high voltage electronics and power semiconductors, such as diodes, FETs, and IGBTs, as well as other components and materials in which high voltage, fast response, and precise measurements of voltage and current are required. The 2657A offers the highest power and best low current performance in the industry. It is supported by the industry's most powerful parametric characterization software platforms to grow with you as your applications evolve.

The 2657A offers highly flexible, four-quadrant voltage and current source/load coupled with precision voltage and current meters. It can be used as a:

- Semiconductor characterization instrument
- V or I waveform generator
- V or I pulse generator
- Precision power supply with V and I readback
- True current source
- Digital multimeter (DCV, DCI, ohms, and power with 6½-digit resolution)
- Precision electronic load

### Key Features

- Source or sink up to 180 W of DC or pulsed power ( $\pm 3000$  V @ 20 mA,  $\pm 1500$  V @ 120 mA).
- 1 fA low current resolution.
- Dual 22-bit precision ADCs and dual 18-bit 1  $\mu$ s per point digitizers for high accuracy and high speed transient capture.
- Fully TSP® compliant for easy system integration with Series 2600B System SourceMeter models.
- Combines a precision power supply, current source, DMM, arbitrary waveform generator, V or I pulse generator, electronic 18-bit load, and trigger controller – all in one instrument.

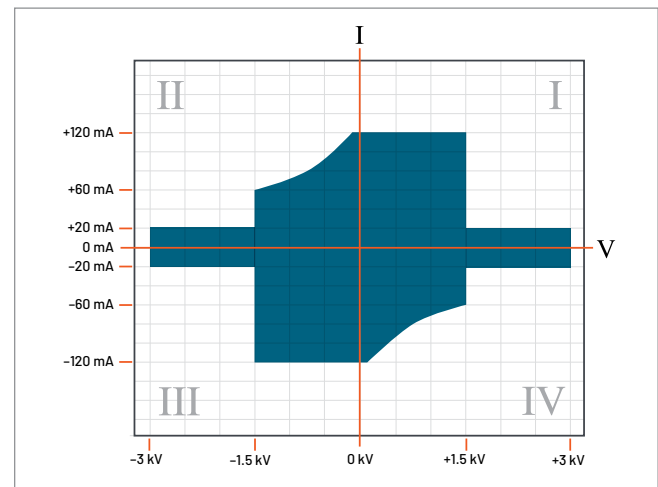

The 2657A can source or sink up to 3000 V @ 20 mA or 1500 V @ 120 mA.

Ihr Ansprechpartner /  
Your Partner:

dataTec AG  
E-Mail: [info@datatec.eu](mailto:info@datatec.eu)  
>>> [www.datatec.eu](http://www.datatec.eu)

**dataTec**

## Typical Applications


- Power semiconductor device characterization and testing
- Characterization of GaN, SiC, and other compound materials and devices
- Breakdown and leakage testing to 3 kV
- Characterization of sub-millisecond transients

## Two Measurement Modes: Digitizing or Integrating

Precisely characterize transient and steady-state behavior, including rapidly changing thermal effects, with the two measurement modes in the 2657A. Each mode is defined by its independent analog-to-digital (A/D) converters.

The digitizing measurement mode provides speeds up to 1  $\mu$ s per sample. The dual 18-bit digitizers allow you to capture voltage and current transients simultaneously. In the integrating measurement mode, the dual 22-bit integrating analog to digital converters allow more precise measurement of voltage and current. Two A/D converters are used with each measurement mode, one for current and the other for voltage, that run simultaneously for accurate source readback that does not sacrifice test throughput.


The dual high speed A/D converters sample as fast as 1  $\mu$ s per point, enabling full simultaneous characterization of both voltage and current.

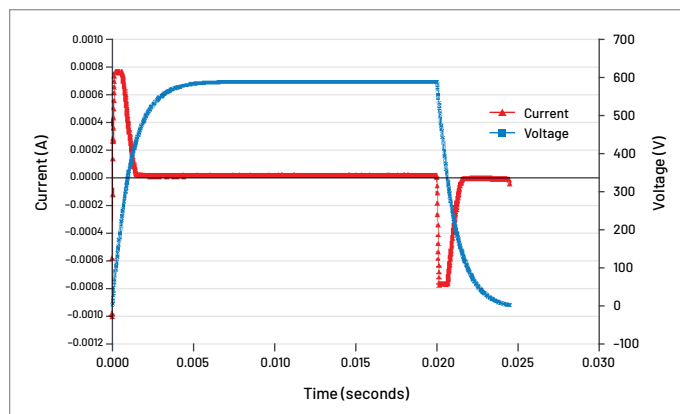

The dual high speed A/D converters sample as fast as 1  $\mu$ s per point, enabling full simultaneous characterization of both voltage and current.

## Expansion Capabilities

Through TSP-Link Technology technology, the 2657A can be linked with Series 2600B SMU instruments to form a larger integrated system with up to 32 nodes. Precision timing and tight channel synchronization are guaranteed with built-in 500 ns trigger controllers. The fully isolated, independent channels of the SourceMeter SMU instruments make true SMU-per-pin testing possible.

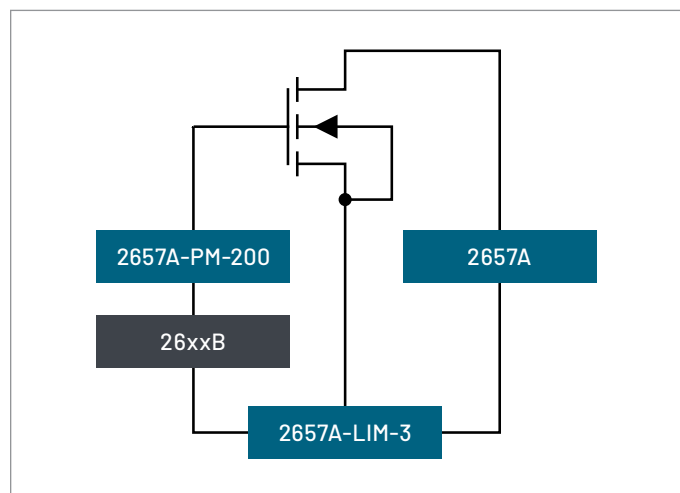

The 2657A can be combined with Series 2600B and 4200-SCS SMU instruments to support multi-terminal test capability. The 2657A-PM-200 Protection Module and 2657A-LIM-3 Low Interconnect Module make it easier to connect multiple instruments to a probe station safely (not required for connecting to the 8010 High Power Device Test Fixture).

## High Power Device Test Fixture

The 8010 High Power Device Test Fixture provides safe and easy connections for testing packaged high power devices at up to 3000 V or 100 A. The 8010 provides connections for a high voltage SourceMeter SMU instrument (2657A), one or two high current SourceMeter SMU instruments (2651A), and three low power SourceMeter SMU instruments (Series 2600B or 4200-SCS SMU instruments). This allows devices with two terminals (diodes) or three terminals (transistors) or even four or five terminals to be characterized safely and accurately. The 8010 has full interlock capability for up to six SourceMeter SMU instruments. The 8010 has integrated protection circuits that protect the low voltage SourceMeter SMU instruments from high voltages the 2657A can output should a device fault occur. The 8010 includes both a high current (100 A) and a high voltage (3000 V) test socket.

Various replacement test socket modules are available, including TO-247, TO-220, axial lead, and a blank socket module that allows building a custom socket. In addition to standard banana jumpers, the 8010 has rear-panel scope and thermal probe ports to simplify system integration.




8010 High Power Device Test Fixture.

## Standard Capabilities of Series 2600B SMU instruments

Each 2657A includes all the features and capabilities provided in Series 2600B SourceMeter SMU instruments:

- Flexibility for use as either a bench-top I-V characterization tool or as a building block component of multiple channel I-V test systems.
- ACS Basic Edition software for semiconductor component characterization (optional). ACS Basic Edition now features a "Trace" mode for generating a suite of characteristic curves.
- Keithley's Test Script Processor (TSP) technology supports creating and running custom user test scripts for high speed test automation, as well as creating programming sequences that allow the instrument to operate asynchronously without direct PC control.
- Parallel test execution and precision timing when multiple Series 2600B SMU instruments are connected together in a system.
- LXI Class C compliance.
- 14 digital I/O lines for direct connection to a probe station, component handler, or other automation tools.
- USB port for extra data and test program storage via USB memory device. Instrument Control Start-up Software

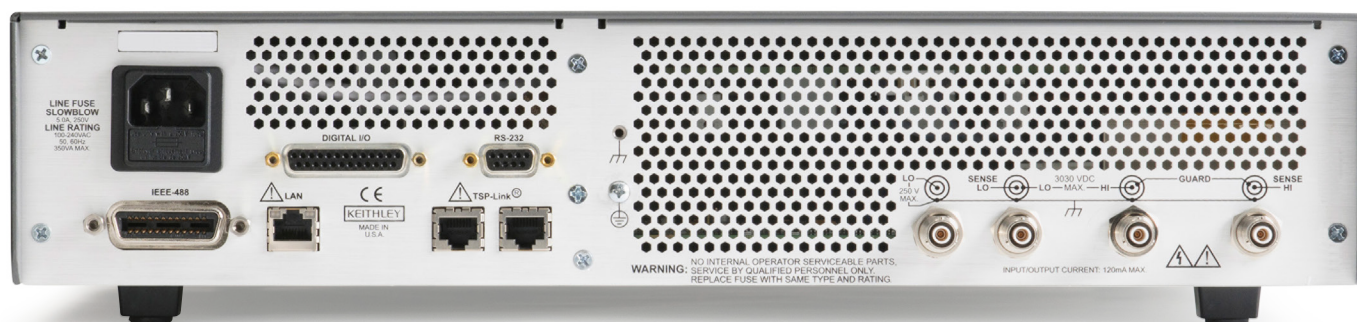

2657A rear panel.



KickStart Start-up Software lets users be ready to make measurements in minutes.

## Instrument Control Start-up Software

KickStart Instrument Control/Start-up Software enables users to start making measurements in minutes without programming. In most cases, users merely need to make some quick measurements, graph the data, and store the data to disk for later analysis in software environments such as Excel. KickStart offers:

- Configure and control up to four SMU instruments for DC or Pulsed I-V test in either the same app, same project, or a combination of the two.
- Create tests by mixing any of these SMU instruments: 2400 Graphical Series, 2400 Standard Series (DC only), 2600B Series, 2651A, 2657A, and 6430 SourceMeter® SMU (DC only) instruments.
- Differentiate SMU instrument channels and their measurement data using labels that are relevant to your device or module.
- Native X-Y graphing, panning, and zooming; screenshot capturing of graphs.
- Spreadsheet/tabular viewing of data; export data for further analysis.
- Annotating of tests; save test setups.
- GPIB, USB 2.0, Ethernet compliance.

## 2657A Condensed Specifications

### Voltage Accuracy Specifications<sup>1</sup>

Range	Source		Measure		
	Programming Resolution	Accuracy $\pm(\% \text{ rdg} + \text{volts})$	Display Resolution	Integrating ADC Accuracy <sup>2</sup> $\pm(\% \text{ rdg} + \text{volts})$	High Speed ADC Accuracy <sup>3</sup> $\pm(\% \text{ rdg} + \text{volts})$
200 V	5 mV	0.03% + 50 mV	100 $\mu$ V	0.025% + 50 mV	0.05% + 100 mV
500 V	10 mV	0.03% + 125 mV	100 $\mu$ V	0.025% + 100 mV	0.05% + 200 mV
1500 V	40 mV	0.03% + 375 mV	1 mV	0.025% + 300 mV	0.05% + 600 mV
3000 V	80 mV	0.03% + 750 mV	1 mV	0.025% + 600 mV	0.05% + 1.2 V

### Current Accuracy Specifications<sup>4</sup>

Range	Source		Measure		
	Programming Resolution	Accuracy $\pm(\% \text{ reading} + \text{amperes} + \text{proportional offset in amperes}). V_o$ is the output voltage.	Display Resolution	Integrating ADC Accuracy <sup>2</sup> $\pm(\% \text{ reading} + \text{amperes} + \text{proportional offset in amperes}). V_o$ is the output voltage.	High Speed ADC Accuracy <sup>3</sup> $\pm(\% \text{ reading} + \text{amperes} + \text{proportional offset in amperes}). V_o$ is the output voltage.
1 nA	30 fA	0.1% + 2 pA + $V_o \times E^{-15}$	1 fA	0.1% + 1.2 pA + $V_o \times E^{-15}$	0.2% + 1.2 pA + $V_o \times E^{-15}$
10 nA	300 fA	0.1% + 5 pA + $V_o \times E^{-14}$	10 fA	0.1% + 5 pA + $V_o \times E^{-15}$	0.2% + 5 pA + $V_o \times E^{-15}$
100 nA	3 pA	0.1% + 60 pA + $V_o \times E^{-13}$	100 fA	0.1% + 60 pA + $V_o \times E^{-13}$	0.2% + 60 pA + $V_o \times E^{-13}$
1 $\mu$ A	30 pA	0.03% + 700 pA	1 pA	0.025% + 400 pA	0.08% + 800 nA
10 $\mu$ A	300 pA	0.03% + 5 nA	10 pA	0.025% + 1.5 nA	0.08% + 3 nA
100 $\mu$ A	3 nA	0.03% + 60 nA	100 pA	0.02% + 25 nA	0.05% + 50 nA
1 mA	30 nA	0.03% + 300 nA	1 nA	0.02% + 200 nA	0.05% + 400 nA
2 mA	60 nA	0.03% + 1.2 $\mu$ A	1 nA	0.02% + 500 nA	0.05% + 1 $\mu$ A
20 mA	600 nA	0.03% + 12 $\mu$ A	10 nA	0.02% + 5 $\mu$ A	0.05% + 10 $\mu$ A
120 mA	3 $\mu$ A	0.03% + 36 $\mu$ A	100 nA	0.02% + 24 $\mu$ A	0.05% + 50 $\mu$ A

1. For temperatures 0° to 18°C and 28° to 50°C, accuracy is degraded by  $\pm(0.15 \times \text{accuracy specification})/^{\circ}\text{C}$ .

2. Derate accuracy specification for NPLC setting <1 by increasing error term. Add appropriate typical percent of range term for resistive loads using the table below.

NPLC Setting	200 V and 500 V Ranges	1500 V and 3000 V Ranges	100 nA Range	1 $\mu$ A to 120 mA Ranges
0.1	0.01%	0.01%	0.01%	0.02%
0.01	0.08%	0.07%	0.1%	0.08%
0.001	0.8%	0.6%	1%	0.7%

3. 18-bit ADC. Average of 1000 samples taken at 100  $\mu$ s intervals.

4. For temperatures 0° to 18°C and 28° to 50°C, accuracy is degraded by  $\pm(0.15 \times \text{accuracy specification})/^{\circ}\text{C}$ . 1 nA to 10  $\mu$ A accuracy is degraded by  $\pm(0.35 \times \text{accuracy specification})/^{\circ}\text{C}$ .

5. Offset (amperes) is typical for 1 nA range.

## SUPPLEMENTAL CHARACTERISTICS

The following specifications are supplemental characteristics that provide additional information about instrument functions and performance. These characteristics are nonwarranted specifications; they describe the typical performance of the 2657A.

## PULSE<sup>6</sup> CHARACTERISTICS

### Pulse Width Programming Resolution

1  $\mu$ s.

### Pulse Width Programming Accuracy

$\pm 10 \mu$ s.

### Pulse Width Jitter

7  $\mu$ s.

**Voltage Source Output Settling Time**

Time required to reach within 1% of final value after source level command is processed on a fixed range<sup>7</sup>  
 $R_L = 10 \text{ M}\Omega$ .

Range	Settling time
200 V	< 5 ms
500 V	< 5 ms
1500 V	< 5 ms
3000 V	< 7 ms


**Current Source Output Settling Time**

Time required to reach within 1% of final value after source level command is processed on a fixed range.

• Values below for  $V = I_{OUT} \times R_{LOAD}$ .

Current Range	$R_{LOAD}$	Settling Time
120 mA	12.5 k $\Omega$	< 5 ms
20 mA	50 k $\Omega$	< 5 ms
2 mA	500 k $\Omega$	< 10 ms
1 mA	1 M $\Omega$	< 5 ms
100 $\mu$ A	10 M $\Omega$	< 15 ms
10 $\mu$ A	100 M $\Omega$	< 20 ms
1 $\mu$ A	1 G $\Omega$	< 200 ms
100 nA	10 G $\Omega$	< 2 s
10 nA	10 G $\Omega$	< 2 s
1 nA	10 G $\Omega$	< 2 s

6. Times measured from the start of pulse to the start off-time; see figure below.

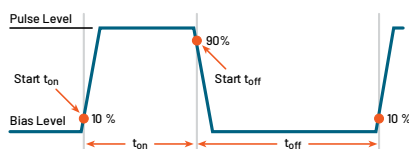

7. With measure and compliance set to the maximum current for the specified voltage range.

**ADDITIONAL SOURCE CHARACTERISTICS**

**Noise 10 Hz to 20 MHz** < 1.2 V peak to peak, < 400 mVRMS. 3000 V range with a 20 mA limit.

**Noise (peak to peak) 0.1 Hz to 10 Hz**

**Voltage** 0.005% of range.

**Current** 0.08% of range.

**Overshoot**

**Voltage** < ±1% for 1500 V and 3000 V ranges. Step size = 10% to 90% of range, resistive load, maximum current limit/compliance.

**Current** < ±1%. Step size = 10% to 90% of range, resistive load. See Current source output settling time for additional test conditions.

**Range Change Overshoot**

**Voltage** < 1% of larger range. Overshoot into a 100 k $\Omega$  load, 20 MHz bandwidth.

**Current** < 5% of larger range.  $I_{OUT} \times R_{LOAD} = 100 \text{ V}$ .

**Guard Offset Voltage** < 4 mV (100 k $\Omega$  guard impedance). Current < 700  $\mu$ A.

**Remote Sense Operating Range<sup>8</sup>** Maximum voltage between HI and SENSE HI = 3 V.  
 Maximum voltage between LO and SENSE LO = 3 V.

**Voltage Output Headroom**

**3000 V Range** Maximum output voltage = 3030 V – (total voltage drop across source leads).



<b>1500 V range</b>	Maximum output voltage = 1515 V – (total voltage drop across source leads).
<b>Overtemperature Protection</b>	Internally sensed temperature overload puts the instrument in standby mode.
<b>Limit (compliance)</b>	Bipolar limit (compliance) set with a single value.
<b>Voltage<sup>9</sup></b>	Minimum value is 20 V; accuracy is the same as voltage source.
<b>Current<sup>10</sup></b>	Minimum value is 100 pA; accuracy is the same as current source.

8. Add 50  $\mu$ V to source accuracy specifications per volt of HI lead drop.

9. For sink operation (quadrants II and IV) without sink mode enabled, add 0.6 percent of limit range to the corresponding voltage source accuracy specifications. Specifications apply with sink mode enabled.

10. For sink operation (quadrants II and IV) without sink mode enabled, add 0.6 percent of limit range to the corresponding current limit accuracy specifications. Specifications apply with sink mode enabled.

## ADDITIONAL CHARACTERISTICS

<b>Contact Check Accuracy</b>	50 $\Omega$ .
<b>Maximum Load Capacitance</b>	Normal mode 100 nF, High-capacitance mode 10 $\mu$ F.
<b>Common Mode Voltage</b>	250 V dc.
<b>Common Mode Isolation</b>	> 1 G $\Omega$ , < 4500 pF.
<b>Sense High Input Impedance</b>	> 100 T $\Omega$ .
<b>Maximum Sense Lead Resistance</b>	1 k $\Omega$ for rated accuracy.
<b>Overrange</b>	101% of source range, 101% of measure range.

## HIGH-CAPACITANCE MODE CHARACTERISTICS<sup>11, 12</sup>

<b>Accuracy Characteristics</b>	Accuracy characteristics are applicable in both normal and high-capacitance modes.								
<b>Voltage Source Output Settling Time</b>	<p>Time required to reach within 1% of final value after source level command is processed on a fixed range for the maximum current limit of the given range<sup>13</sup>. Values below for <math>V_{OUT} = 100</math> V.</p> <table> <tr> <th>Voltage Source Range</th><th>Settling Time with <math>C_{LOAD} = 4.7 \mu F</math></th></tr> <tr> <td>200 V to 500 V</td><td>&lt; 5 ms</td></tr> <tr> <td>1500 V</td><td>&lt; 7 ms</td></tr> <tr> <td>3000 V</td><td>&lt; 30 ms</td></tr> </table>	Voltage Source Range	Settling Time with $C_{LOAD} = 4.7 \mu F$	200 V to 500 V	< 5 ms	1500 V	< 7 ms	3000 V	< 30 ms
Voltage Source Range	Settling Time with $C_{LOAD} = 4.7 \mu F$								
200 V to 500 V	< 5 ms								
1500 V	< 7 ms								
3000 V	< 30 ms								
<b>Current Measure Settling Time</b>	<p>Time required to reach within 1% of final value after voltage source is stabilized on a fixed range. Values below for <math>V_{OUT} = 1</math> kV.</p> <table> <tr> <th>Current Measure Range</th><th>Settling Time</th></tr> <tr> <td>2 mA to 120 mA</td><td>&lt; 100 <math>\mu</math>s</td></tr> <tr> <td>100 <math>\mu</math>A to 1 mA</td><td>&lt; 3 ms</td></tr> <tr> <td>1 <math>\mu</math>A to 10 <math>\mu</math>A</td><td>&lt; 230 ms</td></tr> </table>	Current Measure Range	Settling Time	2 mA to 120 mA	< 100 $\mu$ s	100 $\mu$ A to 1 mA	< 3 ms	1 $\mu$ A to 10 $\mu$ A	< 230 ms
Current Measure Range	Settling Time								
2 mA to 120 mA	< 100 $\mu$ s								
100 $\mu$ A to 1 mA	< 3 ms								
1 $\mu$ A to 10 $\mu$ A	< 230 ms								
<b>Mode Change Delay</b>	<p><b>Current ranges of 100 <math>\mu</math>A and above:</b> 11 ms delay for both in and out of high-capacitance mode.</p> <p><b>Current ranges below 100 <math>\mu</math>A:</b> 250 ms delay into high-capacitance mode. 11 ms delay out of high-capacitance mode.</p>								
<b>Measure Input Impedance</b>	> 30 G $\Omega$ in parallel with 150 pF.								
<b>Voltage Source Range Change Overshoot</b>	< 400 mV + 0.1% of larger range. Overshoot into a 100 k $\Omega$ load, 20 MHz bandwidth.								

11. High-capacitance mode specifications are for dc measurements only and use locked ranges. Autorange is disabled.

12. 100 nA range and below are not available in high-capacitance mode.

13. With measure and compliance set to the maximum current for the specified voltage range.

## MEASUREMENT SPEED CHARACTERISTICS<sup>14</sup>

### Maximum Sweep Operation Rates (operations per second) for 60 Hz (50 Hz):

A/D Converter Speed	Trigger Origin	Measure to Memory (using user scripts)	Measure to GPIB (using user scripts)	Source Measure to Memory (using user scripts)	Source Measure to GPIB (using user scripts)	Source Measure to Memory (using sweep API)	Source Measure to GPIB (using sweep API)
0.001 NPLC	Internal	20000 (20000)	9800 (9800)	7000 (7000)	6200 (6200)	12000 (12000)	5900 (5900)
0.001 NPLC	Digital I/O	8100 (8100)	7100 (7100)	5500 (5500)	5100 (5100)	11200 (11200)	5700 (5700)
0.01 NPLC	Internal	4900 (4000)	3900 (3400)	3400 (3000)	3200 (2900)	4200 (3700)	4000 (3500)
0.01 NPLC	Digital I/O	3500 (3100)	3400 (3000)	3000 (2700)	2900 (2600)	4150 (3650)	3800 (3400)
0.1 NPLC	Internal	580 (480)	560 (470)	550 (465)	550 (460)	560 (470)	545 (460)
0.1 NPLC	Digital I/O	550 (460)	550 (460)	540 (450)	540 (450)	560 (470)	545 (460)
1.0 NPLC	Internal	59 (49)	59 (49)	59 (49)	59 (49)	59 (49)	59 (49)
1.0 NPLC	Digital I/O	58 (48)	58 (49)	59 (49)	59 (49)	59 (49)	59 (49)
High-speed ADC	Internal	38500 (38500)	18000 (18000)	10000 (10000)	9500 (9500)	14300 (14300)	6300 (6300)
High-speed ADC	Digital I/O	12500 (12500)	11500 (11500)	7500 (7500)	7000 (7000)	13200 (13200)	6000 (6000)

### High-speed ADC Burst Measurement Rates:<sup>15</sup>

Burst Length (Readings)	Readings Per Second	Bursts Per Second
100	1,000,000	400
500	1,000,000	80
1000	1,000,000	40
2500	1,000,000	16
5000	1,000,000	8

14. Exclude current measurement ranges less than 1 mA.

15. `smua.measure.adc` must be enabled and the `smua.measure.count` set to the burst length.

### Maximum Single Measurement Rates (operations per second) for 60 Hz (50 Hz):

A/D Converter Speed	Trigger Origin	Measure to GPIB	Source Measure to GPIB	Source Measure Pass/Fail to GPIB
0.001 NPLC	Internal	1900 (1800)	1400 (1400)	1400 (1400)
0.01 NPLC	Internal	1450 (1400)	1200 (1100)	1100 (1100)
0.1 NPLC	Internal	450 (390)	425 (370)	425 (375)
1.0 NPLC	Internal	58 (48)	57 (48)	57 (48)

### Maximum Measurement Range Change Rate

> 4000 per second for > 10  $\mu$ A.

### Maximum Source Range Change Rate

> 250 per second > 10  $\mu$ A.

### Maximum Source Function Change Rate

> 90 per second.

### Command Processing Time

< 1 ms. Maximum time required for the output to begin to change after receiving the `smua.source.levelv` or `smua.source.leveli` command.

## TRIGGERING AND SYNCHRONIZATION CHARACTERISTICS

### Triggering

Trigger In to Trigger Out 0.5  $\mu$ s.

Trigger In to Source Change<sup>16</sup> 10  $\mu$ s.

Trigger Timer Accuracy  $\pm 2$   $\mu$ s.

Source Change<sup>16</sup> after LXI Trigger 280  $\mu$ s.



## SYNCHRONIZATION

**Multi-node Synchronized Source Change<sup>16</sup>**  
 $< 0.5 \mu\text{s.}$


**Single-node Synchronized Source Change<sup>16</sup>**  
 $< 0.5 \mu\text{s.}$

16. Fixed source range with no polarity change.


## SUPPLEMENTAL INFORMATION

<b>Front-panel Interface</b>	Two-line vacuum fluorescent display (VFD) with keypad and navigation wheel
<b>Display</b>	Show error messages and user-defined messages. Display source and limit settings. Show current and voltage measurements. View measurements stored in dedicated reading buffers.
<b>Keypad Operations</b>	Change host interface settings. Save and restore instrument setups. Load and run factory and user-defined test scripts that prompt for input and send results to the display. Store measurements into dedicated reading buffers.
<b>Programming</b>	Embedded Test Script Processor (TSP™) accessible from any host interface; responds to high-speed test scripts comprised of remote commands and statements (for example, branching, looping, and math); able to execute test scripts stored in memory without host intervention.
<b>Minimum User Memory Available</b>	16 MB (approximately 250,000 lines of TSP code).
<b>Reading Buffers</b>	Nonvolatile memory uses dedicated storage areas reserved for measurement data. Reading buffers are arrays of measurement elements. Each element can store the following items: <ul style="list-style-type: none"> <li>• Measurement</li> <li>• Source setting (at the time the measurement was taken)</li> <li>• Measurement status</li> <li>• Range information</li> <li>• Timestamp</li> </ul> Reading buffers can be filled using the front-panel STORE key and retrieved using the RECALL key or host interface.
<b>Buffer Size, with Timestamp and Source Setting</b>	$> 60,000$ samples.
<b>Buffer Size, without Timestamp and Source Setting</b>	$> 140,000$ samples.
<b>Timer</b>	
<b>Timer</b>	Free-running 47-bit counter with 1 MHz clock input. Reset each time instrument power is turned on. If the instrument is not turned off, the timer is automatically reset to zero (0) every four years.
<b>Timestamp</b>	TIMER value is automatically saved when each measurement is triggered.
<b>Resolution</b>	$1 \mu\text{s.}$
<b>Timestamp Accuracy</b>	$\pm 100$ ppm.

## Digital I/O Interface

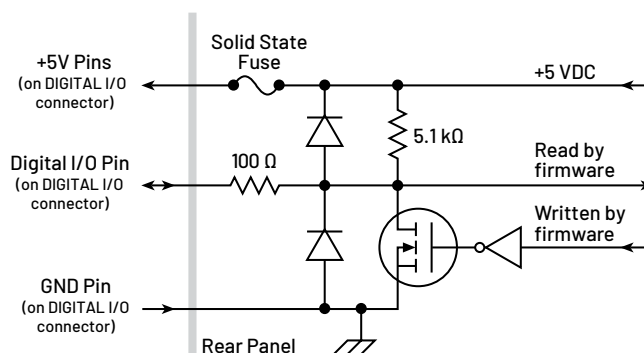

<b>Connector</b>	25-pin female D.
<b>Input/Output Pins</b>	14 open drain I/O bits.
<b>Absolute Maximum Input Voltage</b>	5.25 V.
<b>Absolute Minimum Input Voltage</b>	-0.25 V.
<b>Maximum Logic Low Input Voltage</b>	0.7 V, +850 $\mu$ A.
<b>Minimum Logic High Input Voltage</b>	2.1 V, +570 $\mu$ A.
<b>Maximum Source Current (flowing out of digital I/O bit)</b>	+960 $\mu$ A.
<b>Maximum Sink Current At Maximum Logic Low Voltage (0.7 )</b>	-5.0 mA.
<b>Absolute Maximum Sink Current (flowing into digital I/O pin)</b>	-11 mA.
<b>5 V Power Supply Pin</b>	Limited to 250 mA, solid-state fuse protected.
<b>Safety Interlock Pin</b>	Active high input > 4.0 V at 50 mA must be externally applied to this pin to allow the high-voltage output to operate. Connect the 5 V output and the interlock input of the 25-pin digital I/O connector on the back of the 2657A to the switch in your fixture. The output will be disabled when the interlock signal is < 4.0 V. Absolute maximum input is -0.4 V to +6.0 V.

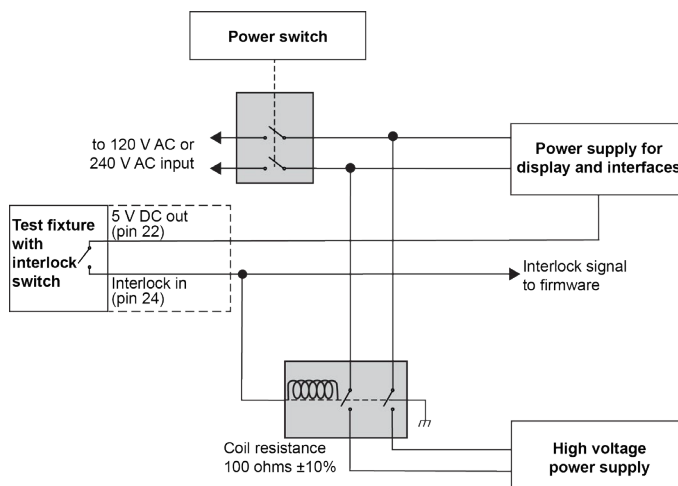

## General Specifications

<b>IEEE-488</b>	IEEE Std 488.1 compliant. Supports IEEE Std 488.2 common commands and status model topology.
<b>RS-232</b>	Baud rates from 300 bps to 115,200 bps. Programmable number of data bits, parity type, and flow control (RTS/CTS hardware or none). When not programmed as the active host interface, the 2657A can use the RS-232 interface to control other instruments.
<b>Ethernet</b>	RJ-45 connector, LXI version 1.4 Core 2011, 10/100Base-T, Auto-MDIX.
<b>LXI compliance</b>	LXI version 1.4 Core 2011.
<b>Expansion interface</b>	The TSP-Link™ expansion interface allows TSP-enabled instruments to trigger and communicate with each other.
<b>USB File System</b>	USB 2.0 Host: Mass storage class device.
<b>Power supply</b>	100 V ac to 240 V ac, 50 Hz or 60 Hz, 350 VA maximum.
<b>Cooling</b>	Forced air; side and top intake and rear exhaust.
<b>Warranty</b>	1 year.
<b>EMC</b>	Conforms to European Union EMC Directive.
<b>Safety</b>	NRTL listed to UL 61010-1:2012 Ed.3+R:16Nov2018 and UL 61010-2-030:2018 Ed.2. Conforms to European Union Low Voltage Directive.
<b>Environment</b>	For indoor use only.
<b>Altitude</b>	Maximum 2000 m (6562 ft) above sea level.
<b>Operating</b>	0 °C to 50 °C, 70% relative humidity up to 35 °C; derate 3% relative humidity/°C, 35 °C to 50 °C.
<b>Storage</b>	-25 °C to 65 °C.
<b>Dimensions</b>	<b>Rack Mount:</b> 89 mm high × 435 mm wide × 630 mm deep (3.5 in. × 17.1 in. × 24.8 in.). <b>Bench Configuration (with handle and feet):</b> 104 mm high × 483 mm wide × 630 mm deep (4.1 in. × 19 in. × 24.8 in.).
<b>Weight</b>	10.7 kg (23.5 lb).

Specifications are subject to change without notice.

## Ordering Information

<b>2657A</b>	High Power System SourceMeter SMU Instrument Cables must be purchased separately. Please contact your local sales office for configuration assistance.
<b>8010</b>	High Power Device Test Fixture

## Supplied Accessories

<b>7709-308A</b>	Digital I/O and Interlock Connector
<b>17469460X</b>	TSP-Link/Ethernet Cable
	Rack Mount Kit
<b>Documentation</b>	Available at <a href="http://www.tektronix.com">www.tektronix.com</a>

## Software Available

<b>KickStart</b>	Instrument Control Software
<b>LabVIEW and IVI Drivers</b>	Available at <a href="http://www.tek.com">www.tek.com</a>
<b>TSP Toolkit Software</b>	Available at <a href="http://www.tek.com">www.tek.com</a>

## Available Accessories

<b>2657A-LIM-3</b>	Low Interconnect Module
<b>2657A-PM-200</b>	200 V Protection Module
<b>SHV-CA-553-x</b>	High Voltage Triax to SHV Cable (1, 2, 3 m)
<b>HV-CA-554-x</b>	High Voltage Triax to Triax Cable (1, 2, 3 m)
<b>HV-CA-571-3</b>	High-Voltage Triaxial Panel-Mount Cable
<b>HV-CS-1613</b>	High Voltage Triax Feedthrough Connector

### Accessories Supplied with the 8010

<b>CA-558-2</b>	25-pin D-sub Interlock Cable for 26xxA
<b>CA-560-x</b>	4 mm Black and Red Banana Cables, 8 in.
<b>CA-562-x</b>	6 mm Black and Red Banana Cables, 10 in.
<b>CA-563</b>	BNC to Banana Cable, 9.5 in.
<b>CA-568-120</b>	Safety Earth Ground Cable

## Contact Information:

Australia 1 800 709 465  
Austria\* 00800 2255 4835  
Balkans, Israel, South Africa and other ISE Countries +41 52 675 3777  
Belgium\* 00800 2255 4835  
Brazil +55 (11) 3530-8901  
Canada 1 800 833 9200  
Central East Europe / Baltics +41 52 675 3777  
Central Europe / Greece +41 52 675 3777  
Denmark +45 80 88 1401  
Finland +41 52 675 3777  
France\* 00800 2255 4835  
Germany\* 00800 2255 4835  
Hong Kong 400 820 5835  
India 000 800 650 1835  
Indonesia 007 803 601 5249  
Italy 00800 2255 4835  
Japan 81 (3) 6714 3086  
Luxembourg +41 52 675 3777  
Malaysia 1 800 22 55835  
Mexico, Central/South America and Caribbean 52 (55) 88 69 35 25  
Middle East, Asia, and North Africa +41 52 675 3777  
The Netherlands\* 00800 2255 4835  
New Zealand 0800 800 238  
Norway 800 16098  
People's Republic of China 400 820 5835  
Philippines 1 800 1601 0077  
Poland +41 52 675 3777  
Portugal 80 08 12370  
Republic of Korea +82 2 565 1455  
Russia / CIS +7 (495) 6647564  
Singapore 800 6011 473  
South Africa +41 52 675 3777  
Spain\* 00800 2255 4835  
Sweden\* 00800 2255 4835  
Switzerland\* 00800 2255 4835  
Taiwan 886 (2) 2656 6688  
Thailand 1 800 011 931  
United Kingdom / Ireland\* 00800 2255 4835  
USA 1 800 833 9200  
Vietnam 12060128

\* European toll-free number. If not accessible, call: +41 52 675 3777

Rev. 02.2022

The logo for dataTec, featuring the word "data" in a lowercase sans-serif font and "Tec" in a stylized, italicized lowercase sans-serif font, both in white on a red rectangular background.

Mess- und Prüftechnik. Die Experten.

**Ihr Ansprechpartner /  
Your Partner:**

**dataTec AG**

E-Mail: [info@datatec.eu](mailto:info@datatec.eu)

>>> [www.datatec.eu](http://www.datatec.eu)

**KEITHLEY**  
A Tektronix Company

Find more valuable resources at [TEK.COM](http://TEK.COM)

Copyright © Tektronix. All rights reserved. Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specification and price change privileges reserved. TEKTRONIX and TEK are registered trademarks of Tektronix, Inc. All other trade names referenced are the service marks, trademarks or registered trademarks of their respective companies.

011525 SBG 1KW-61475-2

